


A. Side rails

To raise a side rail section,


pull section horizontally out of its location to end-stop and fold it upwards. In order to adjust the height of the side rail, pull the telescopic part up to the stop.


To lower a side rail section completely,

- 1. Press the two buttons on the inner side of the frame, right above the cross-member, so that the height-adjustable side rail section can be put into its lowest position.
- 2. Operate the (2a) release button labelled "Push" at the bottom of the side rail part and (2b) tilt it horizontally to the side so that it runs parallel to the floor.
- 3. Push the side rail completely under the lying surface.

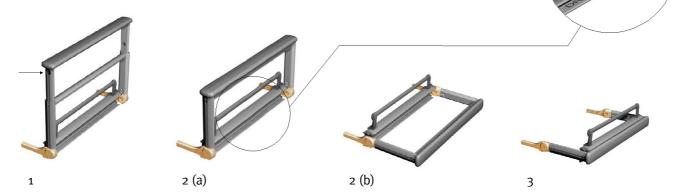

B. Hand control




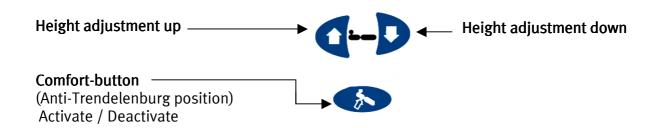

Brief instructions for low height bed model 5380 / 5380 K



C. Caregiver's console with complete lock-out (optional)

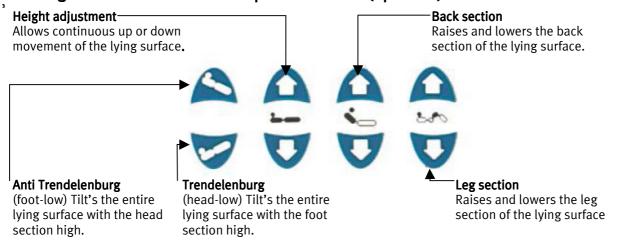

By activating the control lock on the hand control unit, you lock all functions on the hand control. You can still operate the bed by using the caregiver's console.








Deactivate control lock

D. Caregiver's console with single lock-out (optional)

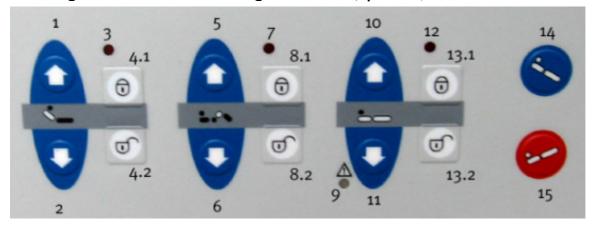

- 1 Back section up
- 2 Back section down
- 3 LED lock of back section *
- 4.1 Lock back section
- 4.2 Unlock back section
- 5 Upper leg section up
- 6 Upper leg section down
- 7 LED lock of upper leg section*
- 8.1 Lock upper leg section

- 8.2 Unlock upper leg section
- 9 LED lowest position of height adjustment
- 10 Height adjustment up
- 11 Height adjustment down
- 12 LED lock of height adjustment *
- 13.1 Lock height adjustment
- 13.2 Unlock height adjustment
- 14 Anti-Trendelenburg position
- 15 Trendelenburg position
- * Glows if function is locked and movement is requested.



Please pay attention to the information in the operating instructions.



Please note that is it not allowed to use the bed for transporting patients.

